

Milk Proteins Intolerance DOT KIT

Beta-Lactoglobulin – Soja

Code: AD-BLSOD

24 Tests - For in vitro use only

1. INTENDED USE

Alphadia Milk Intolerance DOT Kit is an Immunodot kit intended for the detection of IgG antibodies to β -Lactoglobulin (cow's milk) and Soya in human serum.

2. INTRODUCTION

The permeability of the intestinal mucosa to some specific dietary proteins (cow's milk proteins namely) is increased during neonatal period, as the gastrointestinal tract of new-borns is still immature.

Cow's Milk Protein Intolerance (CMPI) is thought to involve a malfunction of immunological tolerance mechanisms at this stage and often appears as the primary cause of a number of disorders frequently observed in young childhood. Hypersensitivity reactions usually occur when switching from mother's breast feeding to cow's milk diet. The symptoms affect the gastrointestinal tract as well the skin, the respiratory tract and may have unsuspected physiological consequences too, such as severe insomnia or hyperagitation. Typically, endoscopy and biopsy examination demonstrate intestinal mucosa alteration.

It is important to distinguish Intolerance from Allergy. Indeed Milk Intolerance is an IgG-mediated immunological process with long-term pathological consequences on the structure of the intestinal mucosa, whereas Milk Allergy is an IgE mediated, short-term hypersensitivity reaction without intestinal involvement.

Anti- β -lactoglobulin IgG antibodies are considered the most specific markers for the diagnosis of CMPI in young children.


Testing for Anti-Soya IgG antibodies is important after a CMPI has been diagnosed and a soya-formulated diet has been set up. Very often a hypersensitivity to soya proteins develops in cow's milk proteins sensitised children.

Alphadia Milk Proteins Intolerance DOT Kit combines elegantly the two serological markers as well as easy handling and cost effectiveness for the reliable differential diagnosis of Food Intolerance to Cow Milk and Soya Protein.

3. PRINCIPLE OF THE TEST

The test is based on the principle of an Enzyme Immunoassay.

The test strip is composed of a membrane fixed on plastic support. During test procedure, the strips are incubated with diluted patients sera. Human antibodies, if present, bind to the corresponding specific antigen(s) on the membrane. Unbound or excess antibodies are removed by washing and AP-conjugated goat antibodies against human IgG are added to the strips. This enzyme conjugate binds to the antigen-antibody complexes. After a second washing step to remove excess conjugate, substrate solution is added. Enzyme activity, if present, leads to the development of purple dots on the membrane pads. The intensity of the coloration is directly proportional to the amount of antibody present in the sample.

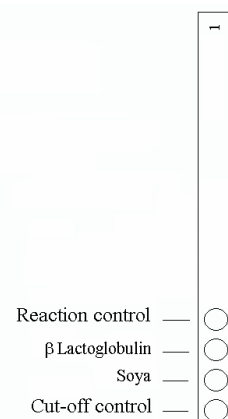

4. KIT CONTENTS

Abbreviations :

TBS = Tris Buffer Saline ; BSA = Bovine Serum Albumin ; MIT = MethylIsoThiazolone ;
AP = Alkaline Phosphatase ; NBT = NitroBlue Tetrazolium ; BCIP = Bromo-Chloro-Indolyl-
Phosphate.

TO BE DILUTED :

(10 X) Wash buffer : **1 x 50 ml** (colourless)
Contains : TBS, Tween ; Preservative : MIT

READY TO USE :

Dot strips : **24 units**
(4 Dots each: 1 reaction control, 2 antigens, 1 cut-off control)

Diluent buffer : **1 x 40 ml** (yellow)
Contains : TBS, BSA, Tween ; Preservative : MIT

Conjugate : **1 x 40 ml** (red)
*Contains : AP-conjugated goat anti-human IgG ;
Preservative : MIT*

Substrate : **1 x 40 ml** (brown bottle, pale yellow solution)
Contains : NBT/BCIP ; Preservative : 0.05 % NaN₃ (sodium azide)

Incubation trays: **3 units**
(with 8 wells for incubation)

5. MATERIAL REQUIRED BUT NOT PROVIDED

Rocking or shaking platform / Micropipettes / Timer / Graduated cylinder /
Distilled or deionised water / Tweezers / Absorbent and/or filter paper

6. STORAGE

The reconstituted Wash Solution is stable for at least one month at 2-8°C.
Reagents and strips can be stored at 2-8°C until the expiry date indicated
on each vial or tube.

Place unused strips back into the provided tube, seal it and store at 2-8°C.
Chromogen/Substrate (NBT/BCIP) shall be stored at 2-8°C.

7. PRECAUTIONS

All reagents are for in vitro diagnostic use only. The kit contains potentially
hazardous components thus avoid contact with skin, eyes or mucosae.
Patient samples shall be handled as potentially infectious. Do not
substitute reagents or mix strips with different batch numbers this may
lead to variations in the results. Avoid touching strips with fingers. Use
tweezers or wear laboratory gloves. Allow reagents and strips to equilibrate
at room temperature before use. Strictly observe incubation times. Handle
Chromogen Substrate (NBT/BCIP) with care in order to avoid any
contamination with Alkaline Phosphatase.

8. SAMPLE COLLECTION, HANDLING AND STORAGE

Samples should be preferentially fresh-collected ones. Sera with debris
should be low speed centrifuged. Blood samples should be collected in dry
tubes or in tubes containing EDTA or heparin. After separation serum
samples shall be used immediately or aliquoted and stored at 2-8°C for
some days or frozen at -20°C for longer periods. Avoid repeated freezing
thawing cycles.

9. ASSAY PROCEDURE

BASIC HANDLING AND TIPS :

The dots are precoloured blue on the strips, ensuring that all antigens have been dotted correctly onto the membrane. This blue coloration disappears during the first step of the procedure. During incubation with the sample a faint pink background coloration appears on the membrane and disappears upon drying at the end of the procedure.

During the procedure, agitation of the incubation tray is necessary to ensure efficient circulation of fluids over the membrane. Any kind of shaking or rocking platform may be used if the amplitude of the movement does not cause spilling out of solutions and cross-contamination between the wells. Agitation speeds ranging from 10 to 60 rpm are suitable, with 20–30 rpm being preferred.

After each filling of the wells with solution, agitate manually the incubation tray to ensure that the strips are completely immersed and to remove air bubbles which may be trapped under the strip. Alternatively, floating strips may be forced into the solution by pushing down (with tweezers or pipette tip) on the upper part of the strip (plastic label zone).

Avoid touching the membrane zone of the strip with fingers, tweezers or pipette tips. Always use the plastic label zone for handling or manipulation. The whole procedure has to be run at room temperature

9.1 Reagents preparation

1. Allow all components to equilibrate at room temperature before use.
2. Dilute the concentrated Wash Buffer 10x with distilled water.

Prepare 15 ml diluted Wash buffer per strip tested

Example: 1,5 ml concentrated wash buffer + 13,5 ml distilled water for one strip.

9.2 TECHNIQUE

1. Place one strip per patient into the wells, blue dots facing up.
2. Add 2 ml Wash Buffer to each well. Incubate (shake) for 10 min.
Upon correct incubation the blue coloration of the dots completely disappears. If not prolong the procedure until the colour of the dots fades completely.
3. Discard solution from the wells.
Remove liquid by slowly inverting the plate. The strips will adhere to the bottom of the wells. Dry the edges of the tray with absorbent paper.
4. Add 1,5 ml Sample Diluent to the wells.
5. Add 10µl patient sample to the wells. Incubate (shake) for 30 min.
Avoid touching the membrane with the pipette tip. Preferentially dispense the sample in the solution over the upper part of the strip (plastic label zone).
Note : Steps 4 and 5 can be combined by pre-diluting the sample in a glass or plastic tube (1,5 ml diluent + 10µl patient sample -> Mix -> Add to the well)
6. Wash 3 x 3 minutes with 1,5 ml Wash Buffer (shake).
Remove liquid from the wells by slowly inverting the plate. The strips will adhere to the bottom of the wells. Dry the edges of the tray with absorbent paper.
7. Add 1,5 ml Conjugate to each well. Incubate (shake) for 30 min.
8. Wash 3 x 3 min. with 1,5 ml Wash Buffer (see 6.)
9. Add 1,5 ml Substrate to the wells. Incubate (shake) for 10 min.
10. Wash 1 x 3 min. with 1,5 ml Wash solution to stop the reaction.
11. Collect the strips from the wells and allow them to dry on absorbent paper.

10. RESULTS INTERPRETATION

10.1 Interpretation

1. Peel off the cover of the adhesive on the back side of each strip and attach strips dots face up onto the marked fields of the interpretation sheet provided with the kit. This will indicate the respective positions of the different controls and antigens on the membrane.
2. Check the first upper Dot (reaction control): it must be positive for all patients.

Only a clearly coloured positive Reaction Control Dot ensures your results are valid and operation was correct and/or kit components were not degraded.

3. Compare the specific antigen Dots to the cut-off Dot which always is the last in order.

The colour intensity of the Antigen Dots is directly proportional to the titer of the specific antibody in the patients sample.

Under optimum conditions and if the sample is free of interfering substances the cut-off dot may be even close to uncoloured. In contrast a highly coloured cut-off Dot indicates a high rate of unspecific binding in the sample.

POSITIVE RESULT: A sample is positive for a specific antibody if the colour intensity of the corresponding Antigen Dot is higher than the intensity of the cut-off Dot.

NEGATIVE RESULT: A sample is negative for a specific antibody if the colour intensity of corresponding Antigen Dot is lower or equal than the intensity of the cut-off Dot.

11. TEST LIMITATIONS

Alphadia Milk Proteins Intolerance DOT Kit is intended for the detection of IgG antibodies to β -Lactoglobulin (cow's milk) and Soya. It serves as an aid for the differential diagnosis and therapy monitoring of Food Intolerance to Cow's milk and Soya Protein. However results have to be interpreted in the light of a complete clinical examination and case history.

12. BIBLIOGRAPHY

- MAY C., L. Remigio and S. Bock (1980)
Usefulness of Measurement of Antibodies in Serum in Diagnosis of Sensitivity to Cow Milk and Soy Proteins in early Childhood.
Allergy, 35 : 301-310
- MAY, C. et al. (1982)
Immunological consequences of feeding infants with cow milk and soya products.
Acta Paediatr. Scand., 71 : 43-51.
- CAVATAIO F. et al. (1996)
Gastroesophageal reflux associated with Cow's Milk Allergy in infants: which diagnostic examinations are useful ?
American Journal of Gastroenterology, 91-6 : 1215-1220.

ALPHADIA
AVENUE VESALE 26
1300 WAVRE – BELGIUM
Tel : +32(0)10 24 26 49
Fax : +32(0)10 24 55 99
e-mail : alphadia@euronet.be